

SPECTRAL PRODUCTS

111 Highland Drive • Putnam CT, 06260 • (860) 928-5834

SMB32Pro 2.8.28

Table of Contents

Warranty and Liability	1
Quick Start Installation Guide	2
System Requirements	3
Requirements for the Hardware	4
Requirements for the Software	4
Check System Package Contents	4
Introduction	5
Software Installation	5
Before You Start	5
Software CD Installation	5
Getting to Know SM32Pro	8
Main Screen	9
Menu Bar	9
Command Button Bar	11
Command Buttons and Dialog Boxes	12
Graph Control Buttons	18
Recording Control Buttons	19
Information Display Area	19
Status Display Bar	19
Quick Access Controls	20
Graph Sliding Bar Controls	20
Special Function Tab	20

Warranty and Liability

This SM product is warranted against defects in material and workmanship for a period of one year from the date of shipment. During the warranty period, Spectral Products will, without charge, repair or replace, at its discretion, the defective product or component parts.

For warranty service or repair, this product must be returned to a service facility designated by Spectral Products (SP). For products returned under warranty, the Buyer shall prepay shipping charges (including shipping charges, duties, and taxes for products returned to SP from another country), and SP will pay for shipping charges to return the product to the Buyer.

This warranty does not apply in the event of misuse or abuse of the product or as a result of unauthorized alterations, modifications or repairs, if the serial number is altered, defaced or removed, the improper or inadequate maintenance by the Buyer, Buyer-supplied software or interfacing, or improper site preparation or maintenance. No other warranty is expressed or implied. SP shall not be liable for any consequential damages, including without limitation, damages resulting from loss of use, as permitted by law.

Quick Start Installation Guide

This quick start guide will walk through the installation of the SM32Pro software package. Please follow the instructions closely to complete the installation. Before beginning, read through this entire guide.

1. Insert the SM installation CD into the appropriate CD-Rom drive. (The installation should begin automatically. If not, open the cd through windows explorer and click on the “**setup.exe**” file to begin the installation manually.)
 - In the case of USB, it is recommended to leave the unit disconnected from the computer until the software has been installed and the system has been rebooted.
2. The first screen displayed requires you to input the user name, company name, and serial number. The full serial number is found on the cover of the SM32Pro.ini diskette that was included in the system package.
3. Accept all the defaults of the next three screens by simply pressing next through each.
 - After these steps are completed, the installer will begin copying the files into the designated folders on the system.
4. When prompted, insert the diskette labeled “SM32Pro.ini” into the appropriate disk drive and click next to continue.
 - If you choose to install this calibration later, you will not be able to run the unit well, or not at all.
5. The installation is now complete. Click finish and manually restart the computer to finish installation of the software.
6. Configuration of boards
 - a. ***For NI users:*** If a National Instruments interface card has been selected, the software will automatically begin the installation of the NIDaq drivers. Follow the default steps and instructions given by the installation procedure to finish and reboot. Once the device has been installed and the computer has been rebooted, the SM32Pro software installation is complete.
 - b. ***For MC users:*** If a Measurement Computing interface card has been selected, the software will automatically open windows explorer to the appropriate location for the driver setup. Run the “Setup.exe” and follow the default steps and instructions given in the InstaCal installation and reboot. Once the device has been installed and the computer has been rebooted, the SM32Pro software installation is complete.
 - c. ***For SM301 users:*** The power connector should be plugged to the detector board before connecting the USB cable to the computer to install the drivers automatically.

Upgrade Installation Guide

This upgrade installation guide will walk through the installation of the SM32Pro upgrade software package. Please follow the instructions closely to complete the installation. Before beginning, read through this entire guide and be sure that the unit has been disconnected from the computer.

Note: Be sure NOT to un-install any previous version of SM32Pro before you upgrade.

1. Insert the SM installation CD into the appropriate CD-Rom drive. (The installation should begin automatically. If not, open the cd through windows explorer and click on the “**setup.exe**” file to begin the installation manually.)
 - In the case of USB, it is recommended to leave the unit disconnected from the computer until the software has been installed and the system has been rebooted.
2. The first screen displayed requires you to input the user name, company name, and serial number. The full serial number is found on the cover of the SM32Pro.ini diskette that was included in the system package.
3. Accept all the defaults of the next three screens by simply pressing next through each.
 - After these steps are completed, the installer will begin copying the files into the designated folders on the system.
4. When prompted, insert the diskette labeled “SM32Pro.ini” into the appropriate disk drive and click next to continue.
 - If you choose to install this calibration later, you will not be able to run the unit well, or not at all.
5. The installation is now complete. Click finish and manually restart the computer to finish installation of the software.
6. Configuration of boards
 - a. ***For NI users:*** If a National Instruments interface card has been selected, the software will automatically begin the installation of the NI Daq drivers. Follow the default steps and instructions given by the installation procedure to finish and reboot. Once the device has been installed and the computer has been rebooted, the SM32Pro software installation is complete.
 - b. ***For MC users:*** If a Measurement Computing interface card has been selected, the software will automatically open windows explorer to the appropriate location for the driver setup. Run the “Setup.exe” and follow the default steps and instructions given in the InstaCal installation and reboot. Once the device has been installed and the computer has been rebooted, the SM32Pro software installation is complete.

System Requirements

Check that your computer meets the minimum requirements for the SM32Pro system.

Requirements for the Hardware

∅ One free slot or port of appropriate type to insert board or connection to the spectrometer

Requirements for the Software

- ∅ Any IBM compatible computer with a 486 processor or higher (Pentium 100 or higher is strongly recommended)
- ∅ A hard drive with at least 50 MB free space
- ∅ A 3 ½ inch high density floppy drive (1.44 MB)
- ∅ A CD-ROM
- ∅ A VGA or compatible display
- ∅ 16 MB RAM (32 MB recommended)
- ∅ A mouse or other pointing device
- ∅ Microsoft Windows® 98, 98SE, ME, NT, 2000, or XP

Check System Package Contents

Check that your SM system package contains all of the required components.

Common system packages contain the following:

- Spectrometer
- A/D board (unless a different interface was requested)
- Cable and Adapter
- Any accessories ordered

****Note: Package contents may vary from unit to unit and order to order. If you have any questions about the contents of your package, please contact the support team referred to in the back of this manual.***

Introduction

SM32Pro is a Windows based operating software designed for use with SP SM series spectrometers. SM32Pro is a true 32-bit application and optimized for SM spectrometer operation control, data acquisition, data manipulation, graphic display, and other features. This user manual will cover the software installation and the various function buttons and features. Please refer to appropriate SM spectrometer hardware user manual for hardware installation and application information.

The SM32PRO.INI file, which is provided together with the SM32Pro, contains instrument specific model information as well as wavelength calibration information. Substitution of the file by inappropriate format may result in a failure in operation. Please contact the factory if such a file is in question.

Software Installation

Before You Start:

It is recommended that the user review the SM spectrometer hardware user manual first to get familiar with the hardware involved. All customers are advised to pay extra attention to the voltage and other electrical ratings associated with the SM spectrometer products to avoid any unnecessary equipment damage.

The following section will describe the SM32Pro software installation procedures. It is recommended that the operating software be installed prior to the hardware installation.

In case a PCMCIA adapter board is needed for a desktop computer, it is recommended to have the adapter board installed first before the start of the SM32Pro software. Please follow the instructions provided by the adapter manufacturer for such an installation.

Software CD Installation:

1. Insert the SM32Pro installation CD into the computer CD ROM.
2. When prompted, enter the instrument serial number as written on the SM spectrometer and then enter the data acquisition code. The code consists of two letters based on the data acquisition board manufacturer and interface types:

Data acquisition board manufacturer:


MANUFACTURER NAMES	CODE
Special data acquisition manufacturer for parallel or serial port type	E
Measurement Computing	B
National Instruments	N
Spectral Products (CVI Laser Corp.)	V

Software Installation (continued):

Data acquisition interface type:

INTERFACE TYPE	CODE
ISA plug-in card	I
PCI plug-in card	P
PCMCIA card	M
USB port	U

For example, the codes will be “EU” for SM240/SM301(-EX) users where a USB interface is used, and “NP” for SM240 customers who are using the National Instruments PCI Interface. The following example shows that the user has an SM240 equipped with a Measurement Computing PCI board.

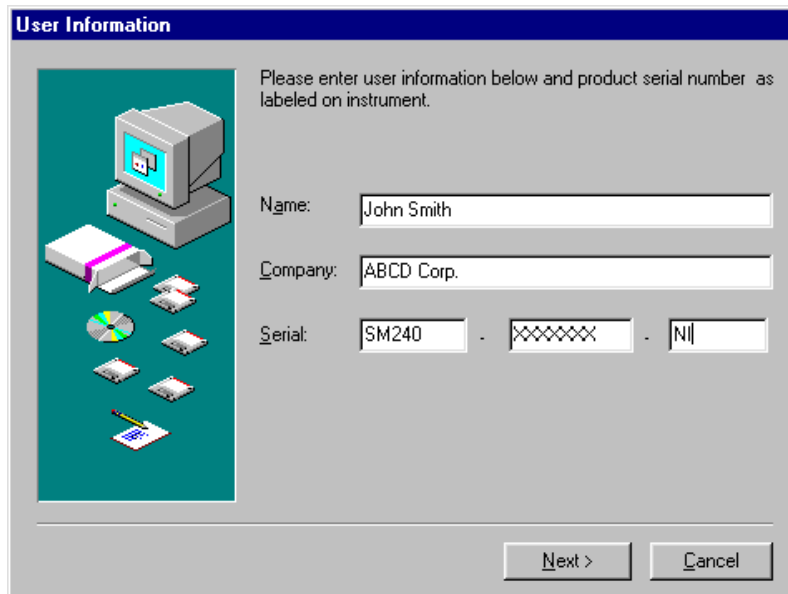

3. Select the applicable software packages to be installed.
4. When prompted to input the initial data file, make sure the supplied disk, which contains the “SM32Pro.ini” file, is inserted into an appropriate disk drive, then press next to copy it to the directory.
5. The selected software package is now installed completely.

***NOTE:** For customers using MC or NI interfaces, you must now install the device drivers.

6. Install the appropriate device drivers by running the “Setup.exe” from the appropriate device driver folder on the SM installation CD. (See quick setup installation guide on page 2 for details)


Software Installation (continued):

7. After the installation of the device driver, shut down the PC and install the board then power back on.

***NOTE:** *If you are using a National Instruments board, the installer will automatically configure the board for you. However, it is suggested that you run the NIMAX utility located in the start menu to verify the boards settings, and that it is working properly.*

A) FOR NATIONAL INSTRUMENTS DATA ACQUISITION BOARD USERS:

If there is a problem with the NI card not being recognized or set properly, you can check the board status using NIMax.exe. You can check if the board is responding properly by right clicking on the board in the **configuration** window and then click on **test resources** or by running the **Test Panel** on the top of the application.

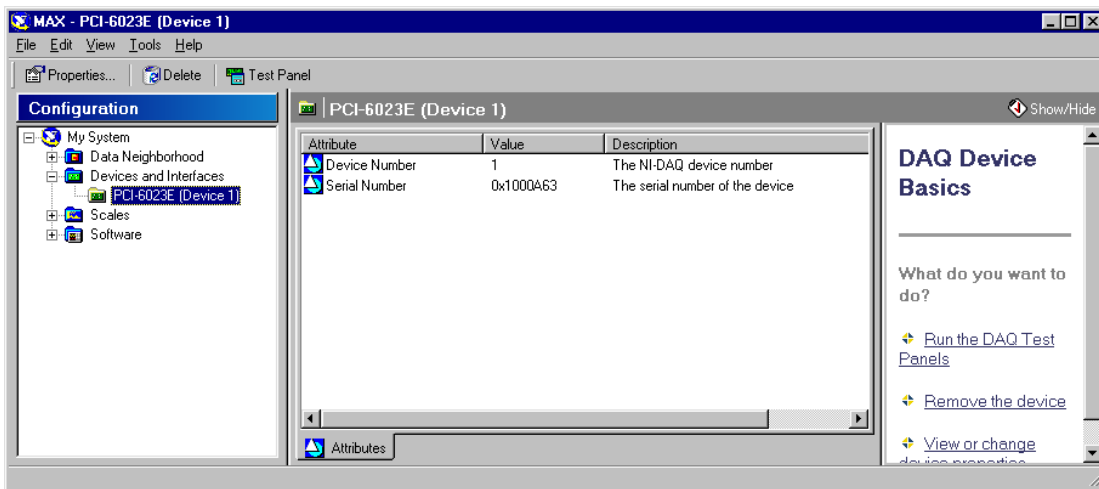

B) FOR MEASUREMENT COMPUTING DATA ACQUISITION CARD USERS:

After the data acquisition board is found and configured by InstaCal, you may simply close the window.

***NOTE:** *If you can see the DEMO board in the list, you have to remove it, and then change the board number on the DAS-1200JR. This can be done by simply right clicking on the appropriate board and choosing the option that would apply (i.e. Right click on the DEMO board and choose “remove board” and be sure to make the “Bd#” for the DAS1200JR “0”)*


Close the InstaCal dialog box. Click on “Finish” in the installer dialog box to complete the installation process.

C) FOR SM301/SM301-EX USERS:


After the installation of the software, please connect the power cable to the unit. And then plug the USB cable to the computer. The drivers will be installed automatically.

***NOTE: If the unit failed to install the drivers automatically, then the drivers should be installed manually. Please open the “device manager” of your OS, and find out the “ADIC Linear Mux Array Controller” on the “Ports” section. If the drivers weren’t installed properly, a question mark or some error mark is on there. Please open it and update the driver. On the process, please choose the “CD drives...” option and continue the process. The installation CD should be in the CD-ROM drive when running this driver updating process.**

When open the software, if the “Com Port” setting is wrong, then the error message window will pop up as below.

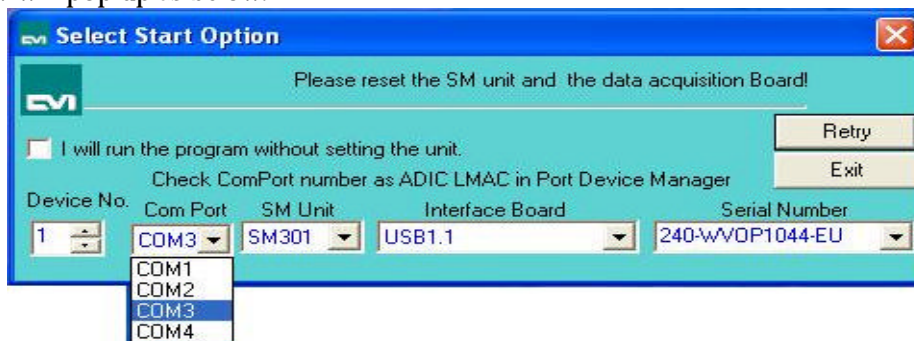

The “Com Port” should be same as that of the installed driver (ADIC Linear Mux Array Controller). Please choose the “Com Port” on the pop-up window. The exact “Com Port” number can be checked on the device manager of the OS as below.

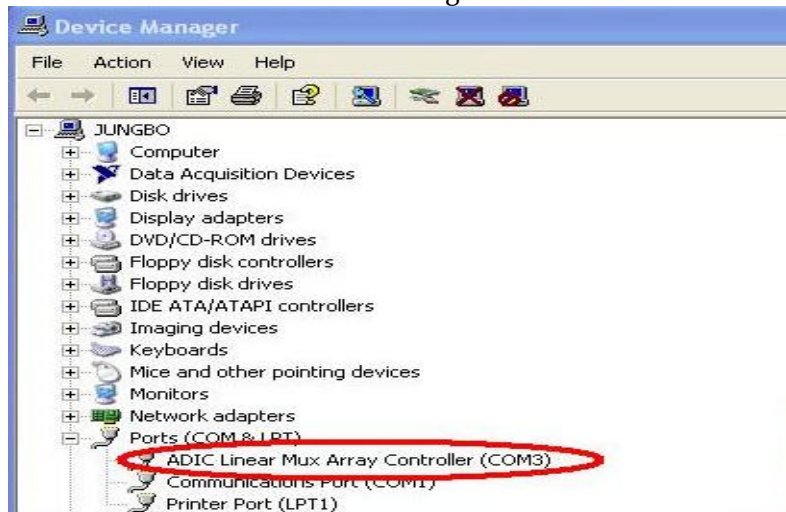


Getting to Know SM32Pro

Main Screen:

The main screen consists of a menu bar, command buttons bar, cursor value and timeline recording display area, graph control buttons bar, project and sample information area, status display area, quick access controls, and a graphic display area.

The graphic display chart consists of two Y scales as well as an X-axis. The Y-axis on the left displays a relative intensity scale in A/D counts in Scope mode while the right Y-axis is defaulted to percentage. The maximum counts shown on the left Y-axis for a 12-bit spectrometer is 4096. When in Scope mode, the X-axis display is in pixel number or in wavelength number. The maximum pixel number is, for example 0 to 2048 for SM240, or it will display the desired wavelength range.

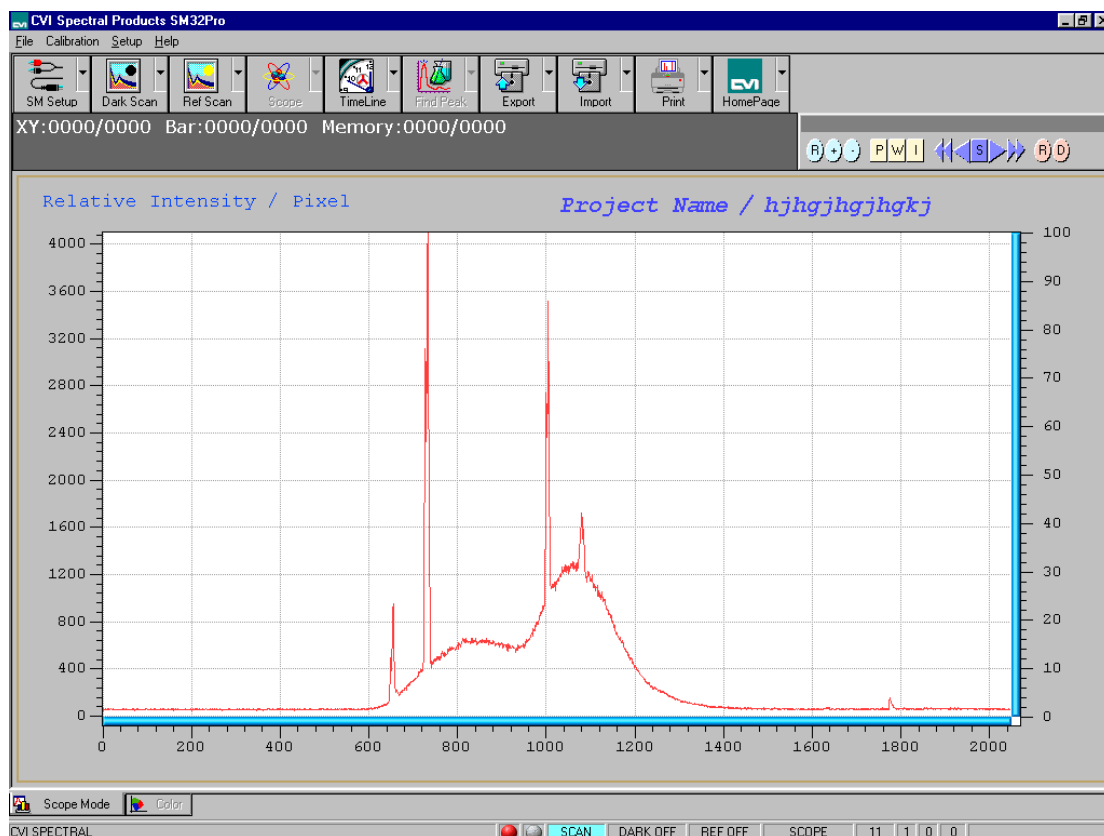

Menu Bar:

CALIBRATION - WAVELENGTH:


Custom wavelength calibration is supported by use of the Calibration tool in Setup>Calibration.

CALIBRATION DIALOG BOX:

Custom wavelength calibration is achieved via the use of the Calibration dialog box. The dialog box consists of a text-editing table for wavelength and pixel value entries, and five different options for loading existing as well as future calibration sets or templates. In calibration mode, all other spectrometer control functions are still supported in the background.

Refresh for Find Peak:

This command button allows the peak finder to update. This is useful when different calibration reference sources are involved in the procedure.

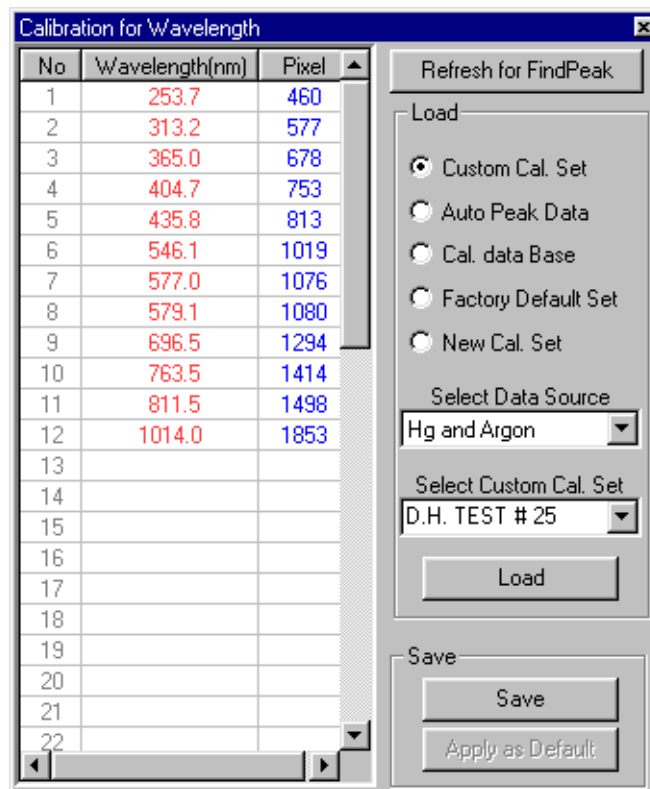

Load options:

Custom Cal Set:

The wavelength calibration set that the SM32Pro utilizes for conversions between different X-axis units is the one labeled as Custom Cal Set. When the Custom Cal Set check box is selected, the display window lists the known wavelength values and corresponding pixel numbers in a tabular format.

Use the Select Custom Cal Set drop down list to highlight the desired wavelength calibration set and then click **Load** to bring the values into the table for adding or subtracting any custom pixel to wavelength reference lines.

Auto Peak Data:

Upon entering the Calibration mode, Peak Finder is automatically started. To use these peak values, (pixels) to generate a new calibration set, select the Auto Peak Data option and click on **Load**. The pixel values that correspond to the found peaks will be copied into the Pixel column for further editing.

The matching known wavelength values can be manually typed into the corresponding cell in the Wavelength column, or click on the Wavelength cell and use the drop down list to select wavelengths from the built-in wavelength database which is comprised of known lines for an HgAr lamp.

Cal Data Base:

This option allows the known wavelength database to be brought into the Wavelength column. Choose a desired wavelength from the Select Data Source drop down list and click on **Load** for the data to be imported.

Factory Default Set:

This option allows the import of the factory created calibration set into the calibration-editing table. Click on **Load** to make the imported data effective.

New Cal Set:

Selecting this option and then clicking **Load** clear the calibration editing table for use to create a new custom calibration set. Wavelengths can be either typed in manually or selected by use of the drop down list as described earlier.

After the creation of the new calibration set type in the desired name into the Select Custom Cal Set field and click on "Save" for the changes to be made. Click on **Apply as Default** to use this particular calibration set as a default.

SETUP - CUSTOMIZE:

By use of the Customize option in the Setup menu, one can customize the print report.

CUSTOMIZE DIALOG BOX:

The Organization name, Operator name and Sample name can be custom changed to be included on the print report.


Command Button Bar

Most of the system operating functions can be realized by use of the command buttons. The command buttons are arranged as general control buttons with embedded pull down dialog boxes, which are opened by clicking on the little arrow on the right side of the button.




Command Buttons and Dialog Boxes

***NOTE:** After working with any dialog boxes described in this or later sections, simply click outside of the dialog box for changes to be effective and to exit.



The SM Setup function allows you to change operating parameters for the spectrometers. Clicking the top right arrow can activate the pull down dialog boxes.

SM SETUP DIALOG BOX:

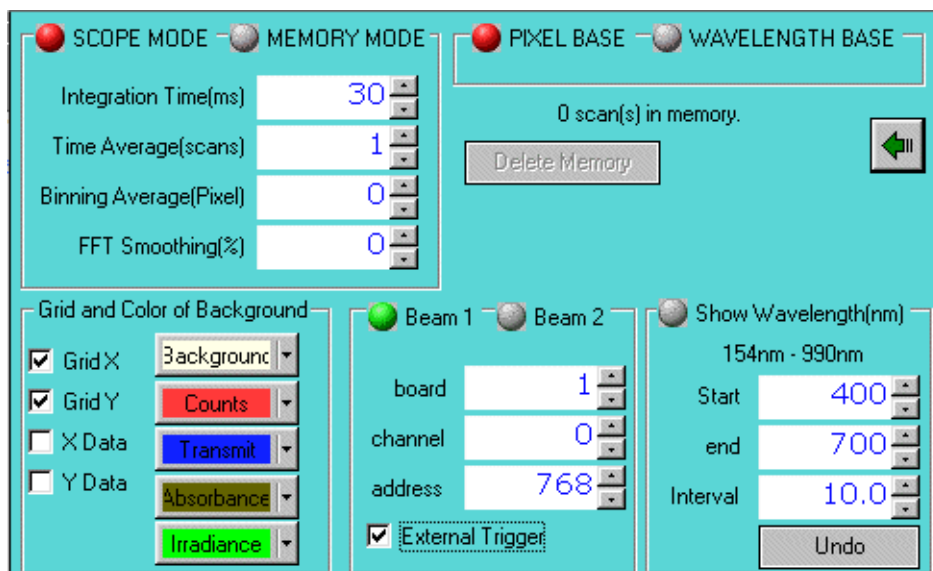

SCOPE MODE is the default-operating mode, which enables the live updating of the measurements.


MEMORY MODE will be entered automatically when a play back operation is performed. The play back of recorded spectra can be achieved by using the **Import** command button.

To exit the repeating play back of recorded spectra, the user needs to use this dialog box to change from **RECORD MODE** back to **SCOPE MODE**.

When the **Pixel Base** display mode is selected wavelength display for clicking W Graph Display Control button will support X-axis in Scope Mode, see also Graph Display Control Buttons. The **Pixel Base** displays wavelength units along the X-axis in appropriate modes. The wavelength increment is the actual wavelength difference between two adjacent sensing pixels.

When **Wavelength Base** is enabled, the wavelengths display mode “W” and the frequency display “I” will not be supported. The only functions that are available in this mode are T/R% or absorbance measurement modes.


When the **External Trigger** box is checked, this will allow you to trigger the spectrometer from an external source. The lowest integration time to use during external triggering is 5ms, but the acquiring and calculation time will be more than 200ms, so the duty cycle for the external signal should be more than the integration time plus 200ms.



The Dark Scan function allows you to perform a dark scan.

**NOTE:* It is recommended that you take a dark scan after the spectrometer integration time is changed. To conduct a dark scan, first block all light from entering the spectrometer. Refer to hardware manual for more information.


DARK SCAN DIALOG BOX:

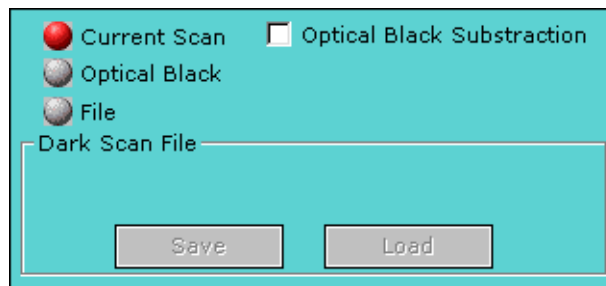

Current Scan: The current scan option is provided to take a dark scan from the current data that is being collected. This dark data can be saved for future dark scanning purposes.


Optical Blank: The optical blank option allows you to use the power emissions from the 32 pixels not used in the collection of data, which only emit dark signal.

File: The file option allows you to use previously saved dark data.



This allows a reference scan to be taken, which is used in T/R% or absorbance measurement for normalization. The pull down dialog box supports several reference scan data sources, from current reference scan, or from a previously saved reference scan data file.

REFERENCE SCAN DIALOG BOX:

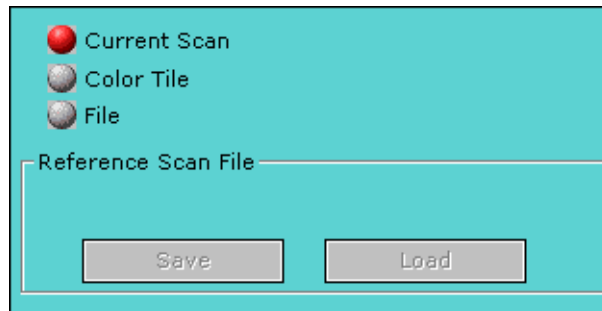

If you chose the **Color Tile** option, the color tile options for **Set Calibration** and **Load Color Tile** will appear in this dialog box.


To use the color tile reference scan, you first have to set the calibration of the specific color tile you wish to use as your reference. Once that is done, the text on the **Reference** button will read **Save Tile**, you will click on this to save the tile calibration as the name you have inputted into the box titled **Project Name**. When you wish to use the calibrated tile as a reference you will choose the calibration for the color tile you wish to use then click on the **Load Color Tile** option. It is now ready to use the color tile. This function is used as a substitute for a white reference scan.

***NOTE:** *The reference scan is required for %T and %R measurements. Reference materials are essential for accurate measurement results to be obtained in different measurement modes and wavelength regions. Refer to hardware manual for more information.*




This indicates the current measurement/display being displayed. The button is enabled only after the dark and reference scans are taken. Click on the button when it is enabled to change between regular scope mode, T/R%, absorbance and irradiance modes.

Display dialog box:

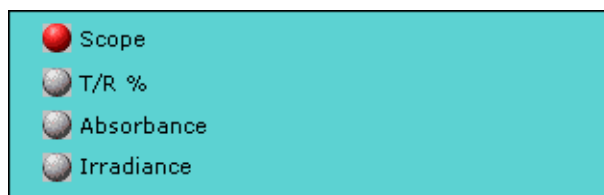

If irradiance is chosen, the irradiance options for absolute or relative measurements and the distance will appear to the right of the selections. There are two kinds of irradiance measurements. The Absolute Irradiance needs to be calibrated by using a calibrated light source. Distance, is the distance from the light source to the unit, and Relative Irradiance needs the calibrations spectrum of the light source, and the color temperature of the light source.



This allows for configurations for automatic sequential spectrum recording at specified time intervals and to specified data files. The pull down dialog box allows for the entry of starting time, ending time, and recording time interval in milliseconds (ms) or seconds (s).

You can choose the duration you want to collect the data by using the time duration function, or by choosing the actual amount of scans you wish to acquire.

TIMELINE DIALOG BOX:

Interval 110 s ms
Start AM 11:25:06 Jun/17/2002
End AM 11:25:06 Jun/17/2002 No 1
File name Project Name
Cancel Record Process Set Ready

The **Timeline** button will become **Ready** after all timeline recording parameters are set. Click on the **Ready** button to start the timed recording process to record spectra within the set duration as shown in the timeline dialog box.

After the start of the Timeline recording the **Ready** button will now be the **Stop** button. Click on the button during recording process to terminate the recording.


***NOTE: The progress of the recording process is updated in the data display area just above the graph display area.**



This allows for the spectral peaks and peak values to be found and displayed. After the peaks are identified, cross hair cursors will appear as you mouse over the peaks. The peak values will be displayed in the **Peak Data** display window.

There are two user configurable parameters in the Find Peak pull down dialog box, which are used by the auto peak finder for peak search. The Peak/Noise Ratio is a value between 0.0 and 10.0 at an increment of 0.1. The higher the ratio the less sensitive the peak finder will be. The Threshold (%) can be set between 0.0 and 100.0.

FIND PEAK DIALOG BOX:

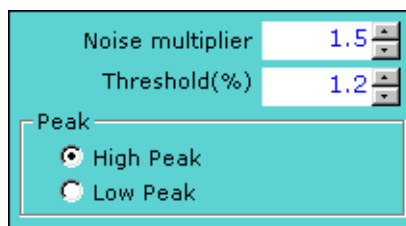


In addition to the peak find, a cursor bar tool is provided. Right click anywhere in the graphics display area and a cross cursor bar will appear with the cross point intercepted by the spectral curve. The cross point values will be displayed in the middle of the display area.

To move the cursor bar around simply place the mouse pointer to the vertical cursor until the pointer changes, which indicates that the cursor bar now is selected for move. Left click the mouse button and drag the cursor to where you desire it. You can also move the cursor bar by pressing the left or right arrow keys on the keyboard. Right click in the graphic display area to exit the cursor bar tool.



This allows export of spectral data to another program via OLE, to an excel file, binary data file, or to a text data file in an ASCII format. The pull down dialog box allows different file formats to be selected.

EXPORT DIALOG BOX:

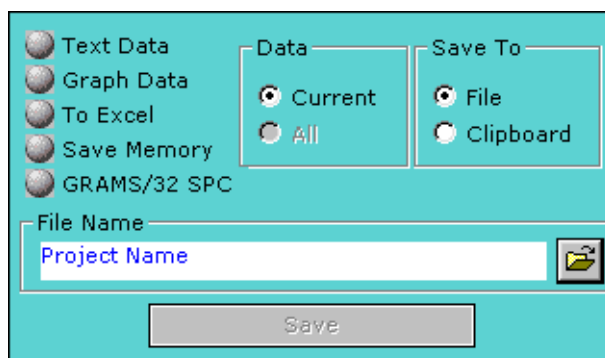


Memory File: When this option is chosen, use the File control button to bring up the file name dialog box for the entry of the file name. The file name will be assigned an extension of **.sdl** for the binary data file format.

Data Table: When this option is chosen, use the File control button to bring up the file name dialog box for the entry of file name. The text data files will have the **.txt** extension. The data values in the file are separated by a space between any pair of data. Data pairs are separated by carriage returns. When the data is exported to an ASCII file, it is set up in a 3 column, tabular format for Pixel, Wavelength, and Intensity.


Excel OLE: When this option is selected the spectral data from the SM32Pro will be exported into a Microsoft Excel spreadsheet. When you click outside the dialog box, the **Export** button becomes the **To Excel** button. Click on the button to start the OLE process for the current spectral data to be exported into the spreadsheet. This spreadsheet includes 2 columns. The first column is for the pixel number or wavelength, depending on which function you are in at the time, and the second column is for the intensity or transmittance data.



This allows for import of previously saved data to be displayed or processed in the current application. This uses a simple dialog box comprised of 2 sections, the file box, and the load button.




This allows for print of the active spectrum. More specific data such as sample source, slit, name, and project name are included in the printout, as well as the peak values for the graph that was printed. These items can be set in the customize option in the program.



This allows for balancing the detector (SM301/SM301EX user only). The detector should be balanced before measuring the sample. Balancing the detector is for setting the stable base line. The input light should be turned off before using this. The pull down dialog box allows setting the TE Cooler On/Off option and the Charge of the Capacitor.

EXPORT DIALOG BOX:

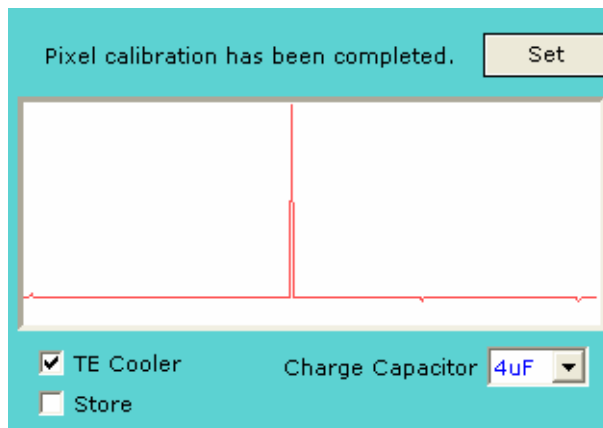

The TE Cooler can be turned on or off with marking the **TE Cooler**. The capacitor charge value for balancing the detector can be set by choosing the value from the **Charge Capacitor** combo box. 1pF, 4pF, 7pF and 10pF are available. For noise purposes it would be desirable to make the sample capacitor larger, but that might result in an unacceptable

loss of signal during the charge sharing. The default value is 4pF and is recommended for use. The **Store** button is an obsolete and has no meaning for the current PbS/PbSe detector. After checking the options, click the **Set** button to start balancing the detector.

Graph Control Buttons

The Graph Control Bar is a convenient utility that puts all of your necessary graph controls at your fingertips.



ZOOMING CONTROLS:



The Zoom control buttons provide zoom Reset (**R**), stepped Zoom In (+), and stepped Zoom Out (-) controls.

Flexible Zoom In can also be achieved by left clicking and holding the mouse button and dragging to draw a Zoom In view window inside the graphic display area around the interested portion.

Clicking the R button does a Complete Zoom Out.

After a graph is zoomed in, two sliding bars will appear for vertical and horizontal scroll control use. Move the mouse pointer to any of the sliding bars until the pointer changes to a double arrow. Click and hold down the left mouse button and slide to view desired spectral display area in the graph.

****NOTE: In addition to the zoom buttons, simply using the mouse pointer can perform zoom in. To do so, left click, drag and draw a rectangular view window around the interested area in the graph.***

X AXIS UNIT CONTROLS:

The display control buttons allow for the selection of spectra to be displayed in pixel (**P**), wavelength in nm (**W**) or inverse centimeters (**I**).

The **W** and **I** display modes apply in T/R% and absorbance measurement modes only if the **Wavelength Base** is selected in SM Setup Dialog Box.

When **Pixel Base** is chosen in the SM Setup Dialog Box, the **W**, wavelength display mode will also be available in Scope measurement mode.

PLAY BACK CONTROLS:



The play back control buttons provide functions when importing and playing back recorded spectra.



This allows for continuous frame-to-frame play back of imported (recorded) spectra in a reverse sequence.



This allows for play back of imported (recorded) spectra in a reverse sequence one frame at a time.



This allows for the termination of continuous play back operation.



This allows for play back of imported (recorded) spectra in a sequence as recorded one frame at a time. In non-recording mode, this button allows a snap spectral shot to be taken each time when there is a click on it.



This allows for continuous play back of imported (recorded) spectra in a sequence as recorded. In non-recording mode (Scope Mode) this button serves as a resume button for continuous acquisition operation.

Recording Control Buttons:



The **R** control will save the current spectrum into memory. The maximum allowable number of spectra to be saved is dependent on the available memory size.

After the manual recording of desired spectra, the **Export** dialog box may be used to assign a file name for the recorded memory files. Thus, the files may be later imported for play back purposes.



The **D** control allows the current displayed spectrum to be deleted from memory manually.

Information Display Area:

XY:0000/0000 Bar:0000/0000 Memory:0000/0000

The display area is located on top of the graphic display and is used for display of mouse pointer positions on X and Y axes in the current spectrum (top left), cursor bar values (middle), timeline recording progress (bottom left), and memory usage (top right). Please also see Peak Finder and Timeline recording, for more information.

Status Display Bar:



The status bar provides information regarding the performed and ongoing operations. These include dark scan status, reference scan status, color measurement status, etc.

Quick Access Controls



The quick access controls are located on the bottom right of the status display and provide easy adjustments to (from left to right) integration time, time average, binning, and FFT filtering settings. Move the mouse pointer to the desired controls and right click to reduce the values or left click to increase the values.


Graph Sliding Bar Controls

There will be two sliding bar controls for vertical and horizontal scroll use when a zoom in tool is applied to the spectral display. Click on the sliding bar with the mouse pointer and hold down while sliding to view different parts of the spectrum.

Special Function Tab

After the dark and reference scans are performed, the Special Function Tab will have Scope and Color tabs enabled. Clicking on the Color tab will enter the color measurement mode. However, the color measurement mode will only be meaningful for spectrometers configured for visible wavelength coverage. To exit the Color mode click on the Scope tab.


Color Analysis Mode:

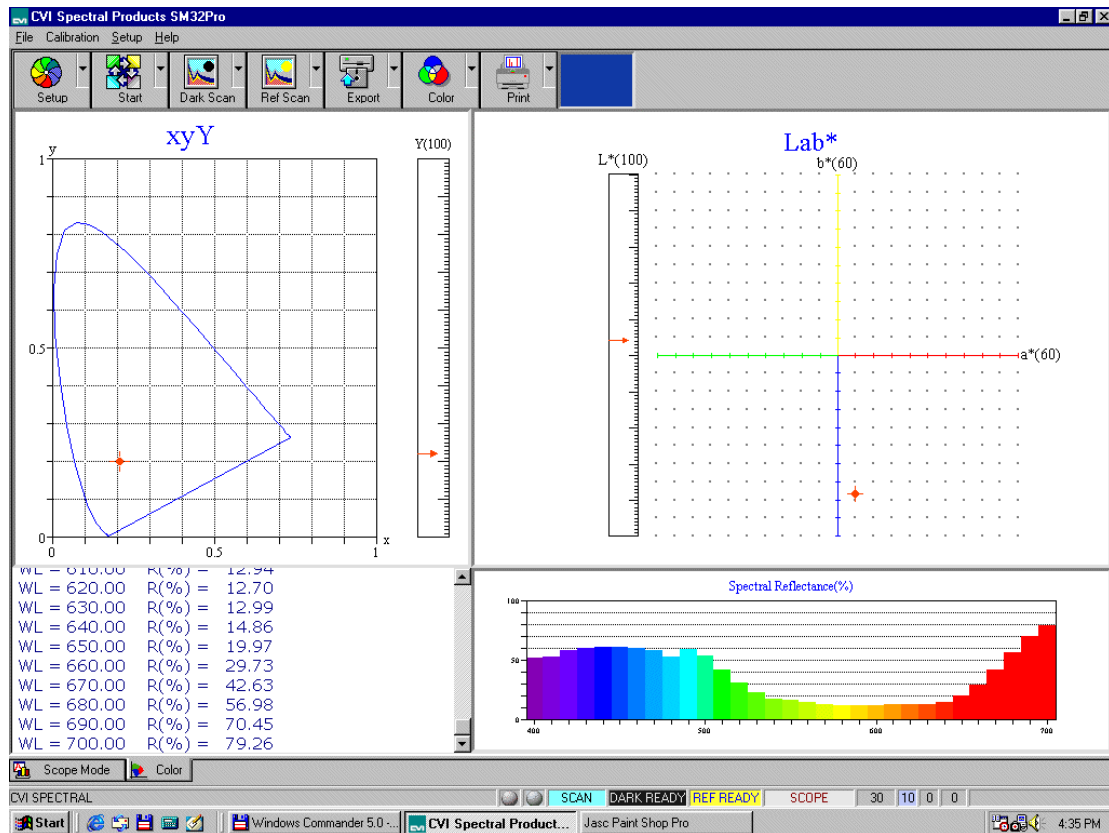


The Color Analysis Mode, as a default, will measure and display color results in the following main screen. The Stop button may be used for obtaining a snap shot and the view of the color values.

COLOR SETUP - CUSTOMIZE:

By use of the Customize option in the Setup menu one can customize the print report.

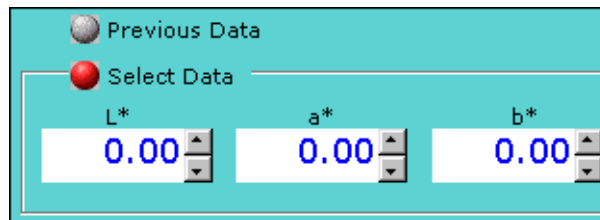

COLOR SOURCE DIALOG BOX:

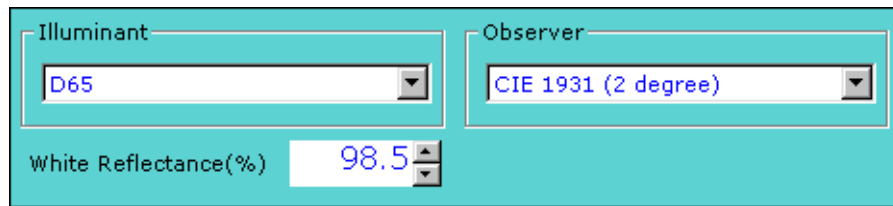

The dialog box is titled "COLOR SOURCE DIALOG BOX:" and contains three main components: an "Illuminant" dropdown menu set to "D65", an "Observer" dropdown menu set to "CIE 1931 (2 degree)", and a "White Reflectance(%)" input field with a numeric value of "98.5".

The pull down dialog box on the top right of the Color command button provides options for the delta E data source. When the **Select Data** option is checked reference L*a*b* values can be entered into the dialog box. The delta E values in the color value display window will now be the color difference between the current measurement results and the entered values. Otherwise, the delta E values displayed will represent the color difference between the current and the previous measurements.

Technical Support

Toll Free: (877) 928-5834
Tel: (860) 928-5834
Fax: (860) 928-2676
Website: <http://www.spectralproducts.com>
Email: support@spectralproducts.com

To help us serve you most efficiently, please collect some information for us before you call:

1. A detailed description of your problem
2. The specific error or error message you received
3. Your system information;
 - a. Software version
 - b. Version of Windows (98, ME, 2000, NT, XP, etc.)
 - c. Unit Serial Number

Our technical staff can be most effective if you are sitting at the computer while consulting technical support.